



| | | | | | | | | | |
|----------|----------|----------|----------|----------|----------|--|--|--|----------|
| | | | | | | | | | 13 Al |
| 22 Ti | 24 Cr | 26 Fe | 27 Co | 28 Ni | 29 Cu | | | | |

M2 Series 5 rematitan® CL

Parameters for GE Additive's Concept Laser M2 Series 5

Data in this material datasheet represents material built with 30 and 60 µm layer thicknesses in an argon atmosphere on a Concept Laser M2 Series 5 single-laser or dual-laser machine and requires build-plate heating. Values listed are typical.



rematitan® CL

Titanium alloy in ELI quality (Grade 23) according to DIN EN ISO 22674 type 4 / DIN EN ISO 9693/ DIN EN ISO 5832-3.

Due to its proven biocompatibility and its long history in the medical industry, it is an established material used for medical/ dental applications.

rematitan® CL is particularly suitable for the manufacture of fixed and removable prosthetic restorations, appliances and metal-ceramic frameworks.

M2 Series 5 rematitan® CL

The parameters for the Concept Laser M2 Series 5 are developed leveraging the performance of other Ti6Al4V Grade 23 parameters. The surface parameter is a 30 µm parameter that produces the best surface roughness, having less than 10 µm without bead blast or shot peening. The productivity parameter has a layer thickness of 60 µm and provides nearly double the productivity of the surface parameter, but still offers very good surface quality. Both parameters have outstanding tensile properties in stress relieved state and meet the DIN EN ISO 22674 type 4/ DIN EN ISO 9693/ DIN EN ISO 5832-3 requirements.



Source: LAC – Laser Add Center GmbH

M2 Series 5 rematitan® CL

With an appropriate approval* rematitan® CL can be used for dental restorations.

Data in this material datasheet represent material built with 30 µm and 60 µm layer thicknesses in an argon atmosphere on a Concept Laser M2 Series 5 single-laser or dual-laser machine and requires build-plate heating. Values listed are typical.

POWDER CHEMISTRY

Ti6Al4V Grade 23 powder chemical composition according to DIN EN ISO 5832-3.

Produced by Dentaureum distributed by GE Additive.

MACHINE CONFIGURATION

- Concept Laser M2 Series 5 (single-laser or dual-laser)
- Argon gas

AVAILABLE PARAMETERS

- **Surface Parameter 235 / 305**** 30 µm layer thickness, rubber recoater
- **Productivity Parameter 236 / 306**** 60 µm layer thickness, rubber recoater


**Productivity optimized version (productivity bundle required)

THERMAL STATES

1. As-Built
2. Stress Relief (SR1)
SR1: 900°C, 1 hour in argon, furnace cooling
3. **Stress Relief (SR2)** - recommended for dental restoration, following the IFU
SR2: 850°C, 1.5 hours in argon, furnace cooling
4. Stress Relief (SR3)
SR3: 730°C, 2 hours in argon, furnace cooling

PARAMETER COMPARISON

■ Surface Parameter SR2 ■ Productivity Parameter SR2



Spider Plot is generated by normalizing typical material data (containing both horizontal and vertical data) against a range defined for each material family. For **Ti6Al4V**, the ranges are as follows: UTS: 600-1100 MPa, 0.2%YS: 500-1000 MPa, Elongation: 0-20 %, Density: 99-100 %, Productivity: 0-60 cm³/h, Surface Quality (all): 50-5 µm

| | Standard | Productivity optimized |
|--|----------------------|------------------------|
| | (cm ³ /h) | (cm ³ /h) |
| Typical build rate ¹ w/coating | 13.1 | 17.1 |
| Theoretical melting rate ² bulk per Laser | 16.8 | 16.8 |

¹Using standard Factory Acceptance Test layout and 2 lasers²Calculated (layer thickness x scan velocity x hatch distance)

PHYSICAL DATA AT ROOM TEMPERATURE

| | Surface Roughness Ra** – Overhang (μm) | | | | Surface Roughness Ra** (μm) | |
|----------|---|-----|-----|---|--------------------------------|---|
| | 45° | 60° | 75° | | H | V |
| Upskin | 8 | 8 | 7 | H | 12 | |
| Downskin | 12 | 8 | 6 | V | 9 | |

| | Relative Density (%) | | Hardness (HV10) | Melting range (°C) | Coefficient of Thermal Expansion CTE 25-500 °C (10 ⁻⁶ /K) |
|----------|----------------------|------|-----------------|--------------------|--|
| | H | V | H | | |
| As-Built | 99.9 | 99.9 | 353 | 1605-1650 | 11.1 |
| SR1 | 99.9 | 99.9 | 334 | -- | -- |
| SR2 | 99.9 | 99.9 | 343 | -- | 10.1 |

Thermal State

TENSILE DATA


Tensile testing done in accordance with ASTM E8 and ASTM E21

Test Temperature:
RT

Thermal State

| | Modulus of Elasticity (GPa) | | 0.2% Yield Strength (MPa) | | Ultimate Tensile Strength (MPa) | | Elongation (%) | | Reduction of Area (%) | |
|----------|-----------------------------|-----|---------------------------|------|---------------------------------|------|----------------|------|-----------------------|----|
| | H | V | H | V | H | V | H | V | H | V |
| As-Built | 111 | 110 | 1145 | 1140 | 1295 | 1270 | 8.0 | 8.5 | 27 | 30 |
| SR1 | 116 | 118 | 920 | 915 | 1010 | 1005 | 15.5 | 15.0 | 44 | 42 |
| SR2 | 114 | 116 | 940 | 945 | 1030 | 1025 | 14.5 | 14.5 | 45 | 44 |
| SR3 | -- | -- | -- | -- | -- | -- | -- | -- | -- | -- |

SEM IMAGES


H: HORIZONTAL (XY) orientation
V: VERTICAL (Z) orientation

* All of the figures contained herein are approximate only. The figures provided are dependent on a number of factors, including but not limited to, process and machine parameters, and the approval is brand specific and/or application specific. The information provided on this material data sheet is illustrative only and cannot be relied on as binding.

** Roughness measurements have been performed according to DIN EN ISO 4287 and DIN EN ISO 4288. In general analysis of the surface quality is strongly dependent on the methodology used and therefore deviations might be observed depending on methodology used. Vertical and horizontal sidewalls have been characterized using a tactile system, overhangs using an optical system.


The platform stability build evaluates porosity, roughness and tensile properties across different positions and orientations. To illustrate the position dependency of the M2 Series 5, the samples were homogenously distributed across the platform on 16 different positions. Regarding surface quality all sides of the specimen, so all orientations with respect to gas flow and optical system, are included in the analysis. Data shown below are dependent on part & print layout as well as batch chemistry variations and thus might deviate from “typical values” given on previous pages.

BUILD JOB DESIGN AND SUMMARIZED DATA (STRESS RELIEF SR1)




| | Sample Size | Mean | St.Dev. | | Sample Size | Mean | St.Dev. |
|--|-------------|-------|---------|-----------------------|-------------|-----------|---------|
| Rel. Density in % | 32 | 99.99 | 0.01 | YM in GPa (H/V) | 16/16 | 115/118 | 2/1 |
| Sidewall Roughness Ra in μm | 64 | 8.7 | 0.9 | YS in MPa (H/V) | 16/16 | 927/933 | 2/6 |
| Upside Roughness Ra in μm (60°) | 64 | 7.3 | 1.8 | UTS in MPa (H/V) | 16/16 | 1019/1020 | 2/2 |
| Downside Roughness Ra in μm (60°) | 64 | 8.4 | 0.8 | Elongation in % (H/V) | 16/16 | 15.7/15.1 | 0.8/0.5 |

RESULTS - RELATIVE DENSITY AND SURFACE QUALITY



RESULTS - MECHANICAL PROPERTIES



Data points represent the mean value, intervals the 95% confidence level.

H: HORIZONTAL (XY) orientation
V: VERTICAL (Z) orientation

| | Standard | Productivity optimized |
|--|----------------------|------------------------|
| | (cm ³ /h) | (cm ³ /h) |
| Typical build rate ¹ w/coating | 26.5 | 39.0 |
| Theoretical melting rate ² bulk per Laser | 40.4 | 40.4 |

¹Using standard Factory Acceptance Test layout and 2 lasers²Calculated (layer thickness x scan velocity x hatch distance)

PHYSICAL DATA AT ROOM TEMPERATURE

| | Surface Roughness Ra** – Overhang (µm) | | | | Surface Roughness Ra** (µm) | |
|----------|---|-----|-----|---|--------------------------------|---|
| | 45° | 60° | 75° | | H | V |
| Upskin | 20 | 17 | 13 | H | 18 | |
| Downskin | 17 | 13 | 9 | V | 10 | |

| | Relative Density (%) | | Hardness (HV10) | Melting range (°C) | Coefficient of Thermal Expansion CTE 25-500 °C (10 ⁻⁶ /K) |
|----------|----------------------|------|-----------------|--------------------|--|
| | H | V | H | | |
| As-Built | 99.9 | 99.9 | 357 | 1605-1650 | 10.9 |
| SR1 | 99.9 | 99.9 | 342 | -- | -- |
| SR2 | 99.9 | 99.9 | 347 | -- | 10.1 |

Thermal State

TENSILE DATA

Tensile testing done in accordance with ASTM E8 and ASTM E21


Test Temperature:

RT

| | Modulus of Elasticity (GPa) | | 0.2% Yield Strength (MPa) | | Ultimate Tensile Strength (MPa) | | Elongation (%) | | Reduction of Area (%) | |
|----------|--------------------------------|-----|------------------------------|------|------------------------------------|------|-------------------|------|--------------------------|----|
| | H | V | H | V | H | V | H | V | H | V |
| As-Built | 113 | 112 | 1115 | 1125 | 1255 | 1275 | 7.0 | 8.0 | -- | -- |
| SR1 | 121 | 118 | 940 | 940 | 1015 | 1015 | 16.0 | 14.5 | -- | -- |
| SR2 | 118 | 115 | 945 | 940 | 1030 | 1030 | 15.0 | 14.0 | 42 | 40 |
| SR3 | 119 | 120 | 1080 | 1075 | 1135 | 1130 | 12.0 | 11.5 | -- | -- |

Thermal State

SEM IMAGES




H: HORIZONTAL (XY) orientation
V: VERTICAL (Z) orientation

* All of the figures contained herein are approximate only. The figures provided are dependent on a number of factors, including but not limited to, process and machine parameters, and the approval is brand specific and/or application specific. The information provided on this material data sheet is illustrative only and cannot be relied on as binding.

** Roughness measurements have been performed according to DIN EN ISO 4287 and DIN EN ISO 4288. In general analysis of the surface quality is strongly dependent on the methodology used and therefore deviations might be observed depending on methodology used. Vertical and horizontal sidewalls have been characterized using a tactile system, overhangs using an optical system.


The platform stability build evaluates porosity, roughness and tensile properties across different positions and orientations. To illustrate the position dependency of the M2 Series 5, the samples were homogenously distributed across the platform on 16 different positions. Regarding surface quality all sides of the specimen, so all orientations with respect to gas flow and optical system, are included in the analysis. Data shown below are dependent on part & print layout as well as batch chemistry variations and thus might deviate from “typical values” given on previous pages.

BUILD JOB DESIGN AND SUMMARIZED DATA (STRESS RELIEF SR1)




| | Sample Size | Mean | St.Dev. | | Sample Size | Mean | St.Dev. |
|--|-------------|-------|---------|-----------------------|-------------|-----------|---------|
| Rel. Density in % | 32 | 99.93 | 0.03 | YM in GPa (H/V) | 16/16 | 117/119 | 3/5 |
| Sidewall Roughness Ra in μm | 64 | 9.5 | 1.0 | YS in MPa (H/V) | 16/16 | 935/940 | 4/5 |
| Upside Roughness Ra in μm (60°) | 64 | 11.7 | 2.0 | UTS in MPa (H/V) | 16/16 | 1025/1024 | 2/3 |
| Downside Roughness Ra in μm (60°) | 64 | 9.6 | 1.5 | Elongation in % (H/V) | 16/16 | 14.2/13.9 | 0.5/1.3 |

RESULTS - RELATIVE DENSITY AND SURFACE QUALITY




RESULTS - MECHANICAL PROPERTIES




Data points represent the mean value, intervals the 95% confidence level.


H: HORIZONTAL (XY) orientation
V: VERTICAL (Z) orientation

As-Built condition, vertical direction

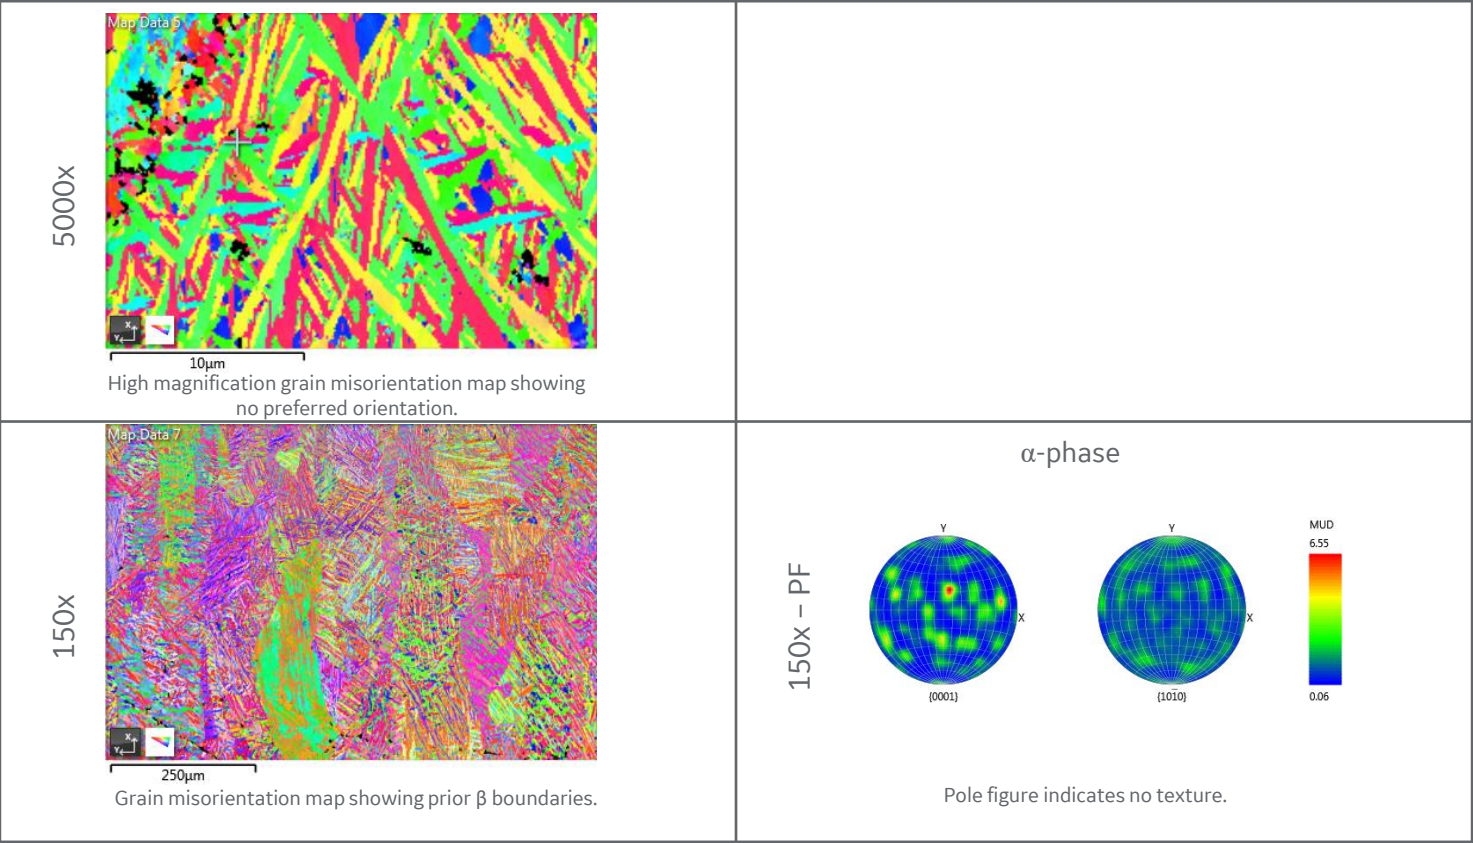

SR1 condition, vertical direction

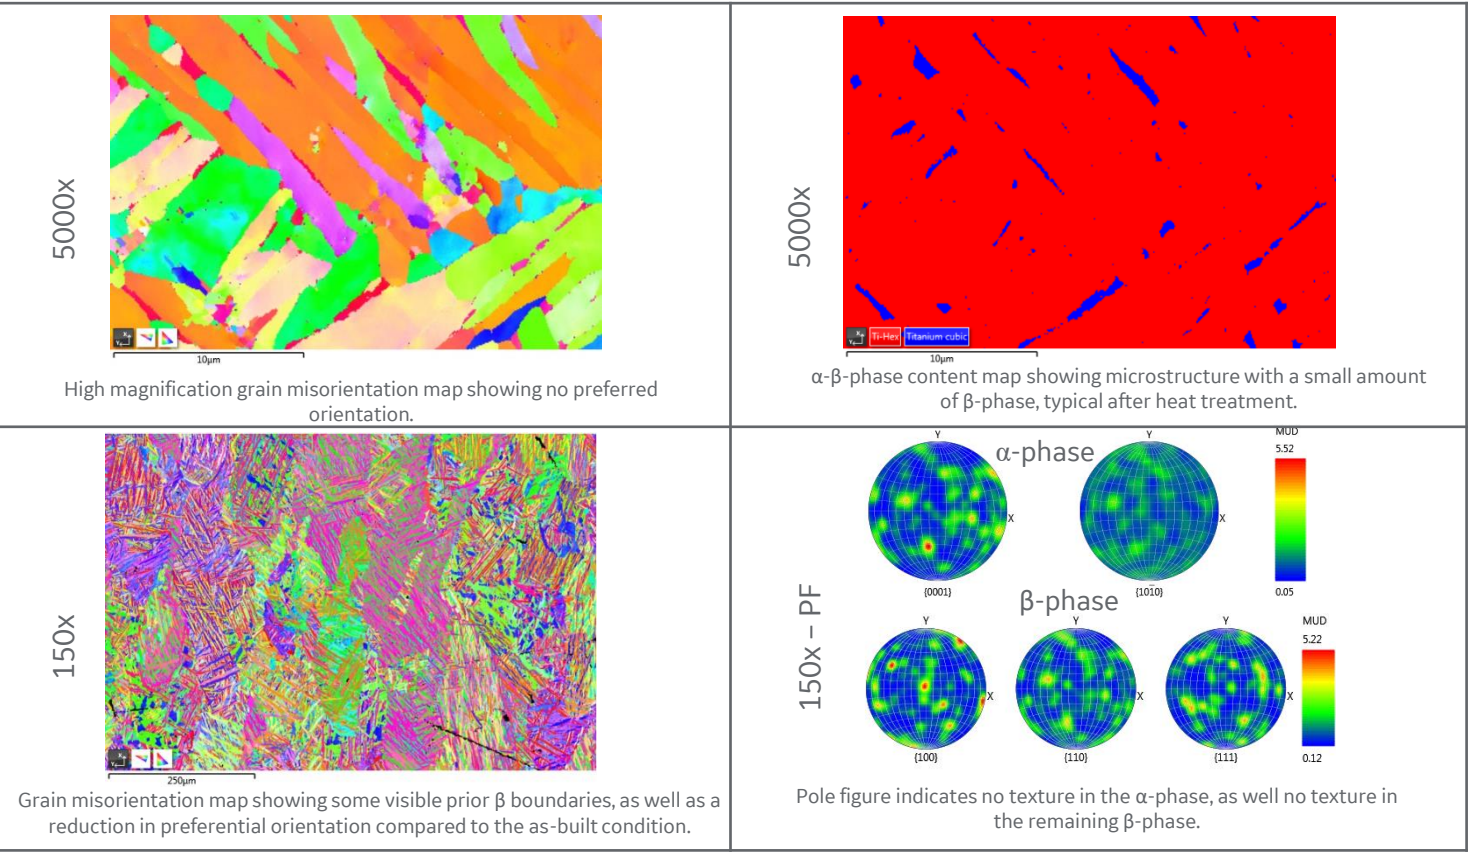



M2 Series 5 rematitan® CL Mesh+ Parameters

Premium+ Parameters for GE Additive's Concept Laser M2 Series 5

Data in this material datasheet represent material built with 30 and 60 µm layer thicknesses and in an argon atmosphere on a Concept Laser M2 Series 5 single-laser or dual-laser machine and requires build-plate heating. Values listed are typical.



rematitan® CL

Titanium shows a high corrosion resistance and proven biocompatibility and has been employed successfully in human implant applications in contact with soft tissue and bone for decades.

Porous (trabecular) structures are very common for AM-manufactured medical implants. The open titanium architecture results in open structures that lead to enhanced osseointegration and allows adjusting the final device characteristics (density, stiffness). It also requires a well-balanced parameter set to optimize the build process fulfilling the productivity and quality requirements.

M2 Series 5 rematitan® CL Mesh+ Parameters

The mesh+ parameters enable the user to design porosity and pore size, as well as interconnectivity of trabecular structures to allow for enhanced initial fixation and bone ingrowth. The parameters further provide the user with an exceptional balance of high grade of detail and high productivity.

The Mesh+ parameters can be used in conjunction with the Concept Laser M2 Series 5 rematitan® CL parameters to create parts with both solid and mesh volumes to create hybrid components.



M2 Series 5 rematitan® CL Mesh+ Parameters

Data in this material datasheet represent material built with 30 and 60 µm layer thicknesses in an argon atmosphere on a Concept Laser M2 Series 5 single-laser or dual-laser machine and requires build-plate heating. Values listed are typical.

POWDER CHEMISTRY

Ti6Al4V Grade 23 powder chemical composition according to DIN EN ISO 5832-3.
Produced by Dentaureum distributed by GE Additive.

MACHINE CONFIGURATION

- Concept Laser M2 Series 5 (single-laser or dual-laser)
- Argon gas


AVAILABLE PARAMETERS

- **Mesh+ Parameter 237 / 307**** 30 µm layer thickness, rubber recoater
 - **Mesh+ Parameter 238 / 308**** 60 µm layer thickness, rubber recoater
- **productivity optimized version (productivity bundle required)

THERMAL STATES

1. As-Built
2. Stress Relief (SR1)
SR1: 900°C, 1 hour in argon, furnace cooling
3. HIP
HIP: 900°C, 2 hours, pressure 100 MPa

PARAMETER COMPARISON



Spider Plot is generated by normalizing typical material data (containing both horizontal and vertical data) against a range defined for each material family. For **Ti6Al4V (mesh parameter)**, the ranges are as follows: Compression UTS (Mesh): 0-110 MPa, Compression YS (Mesh): 0-85 MPa, Density: 0-80%, Productivity: 5-40 cm³/h, Max. Pore Size: 0-600 µm, Strut Thickness: 0-300 µm

| | (cm ³ /h) |
|--|----------------------|
| Theoretical melting rate ² bulk per Laser | 17.5 |

²Calculated (layer thickness x scan velocity x hatch distance)

COMPRESSION STRENGTH OF MESH STRUCTURE**

Compression testing done in accordance with ISO 13314

| | Modulus of Elasticity (Compression) (GPa) | YS (Compression) (MPa) | Compressive Strength (MPa) |
|----------|---|------------------------------|-------------------------------|
| As-Built | 2.2 | 80 | 104 |
| SR1 | 2.5 | 81 | 104 |
| HIP | 2.3 | 76 | 100 |

MESH DIMENSIONS**



| | Mesh porosity (%) | Strut thickness (μm) | Max. pore size (μm) |
|----------|----------------------|-------------------------|------------------------|
| As-Built | 63 | 250 | 480 |

SEM & CAD IMAGES

As-Built

SR1

Vertical (bulk)



CAD

SEM image

Mesh design**




Image shows the post-processed condition

V: VERTICAL (Z) orientation

*All of the figures contained herein are approximate only. The figures provided are dependent on a number of factors, including but not limited to, process and machine parameters, and the approval is brand specific and/or application specific. The information provided on this material data sheet is illustrative only and cannot be relied on as binding.

** Data demonstrating results of special mesh design. Different designs could lead to changes in properties.

| | |
|--|----------------------|
| | (cm ³ /h) |
| Theoretical melting rate ² bulk per Laser | 36.9 |

²Calculated (layer thickness x scan velocity x hatch distance)

COMPRESSION STRENGTH OF MESH STRUCTURE**

Compression testing done in accordance with ISO 13314

| | Modulus of Elasticity (Compression) (GPa) | YS (Compression) (MPa) | Compressive Strength (MPa) |
|----------|---|------------------------------|-------------------------------|
| As-Built | 1.2 | 51 | 60 |
| SR1 | 1.3 | 50 | 60 |
| HIP | 1.3 | 47 | 64 |


MESH DIMENSIONS**

| | Mesh porosity (%) | Strut thickness (µm) | Max. pore size (µm) |
|----------|----------------------|-------------------------|------------------------|
| As-Built | 64 | 240 | 490 |


SEM & CAD IMAGES

Vertical (bulk)

As-Built

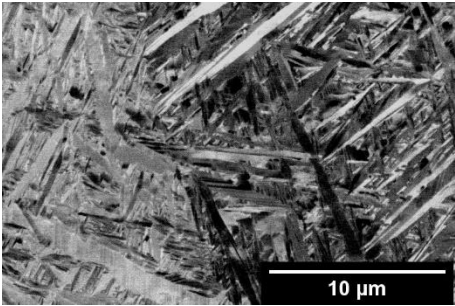


SR1

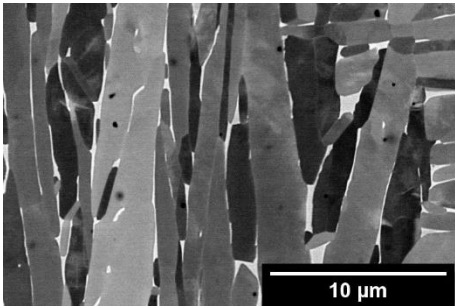

Mesh design**

CAD

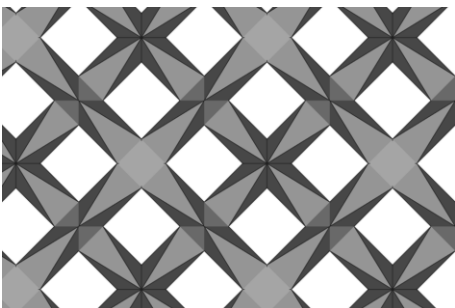

SEM image

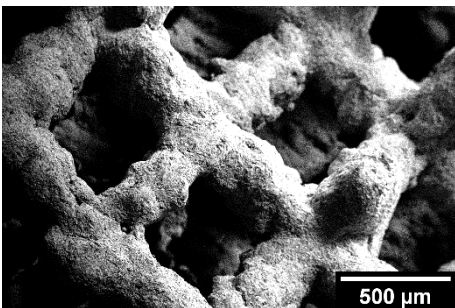


Image shows the post-processed condition

V: VERTICAL (Z) orientation

*All of the figures contained herein are approximate only. The figures provided are dependent on a number of factors, including but not limited to, process and machine parameters, and the approval is brand specific and/or application specific. The information provided on this material data sheet is illustrative only and cannot be relied on as binding.
** Data demonstrating results of special mesh design. Different designs could lead to changes in properties.